REV	DATE	BY	DESCRIPTION	ECO
-	07/20/09	jodell	DRAWING CREATED	F523
A	8-27-09	GJO	UPDATED NOTES AND ADDED SHEET 2 OF 2 WITH FULL SCALE TEMPLATE	F573

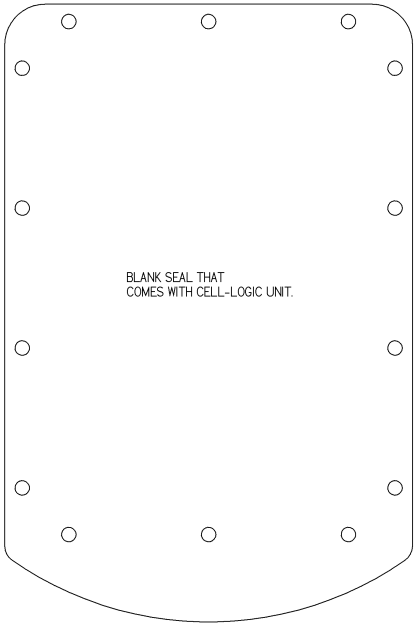

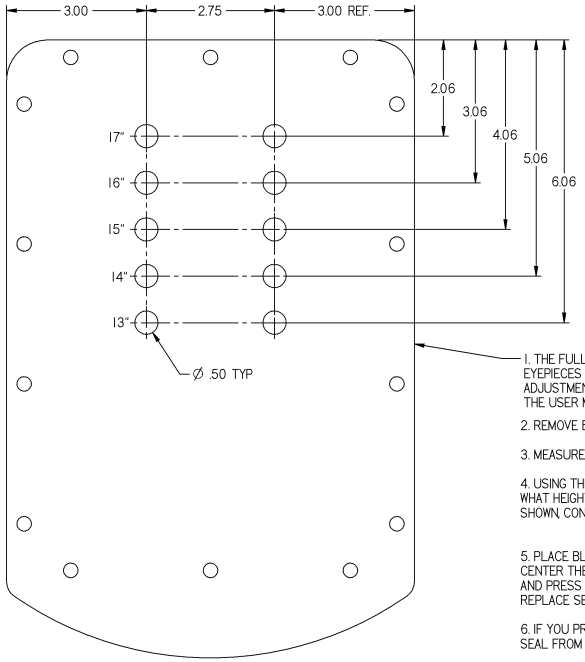

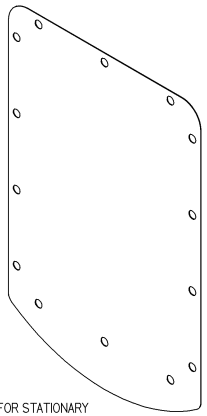

1. THE FULL SCALE (PURE - VU) TEMPLATE ON SHEET 2 OF 2 IS FOR STATIONARY EYEPIECES HEIGHT. FOR STEREOSCOPES WITH FREQUENT EYEPIECE HEIGHT ADJUSTMENTS SELECT A (PURE - VU XL) SEAL FROM APPENDIX D IN THE USER MANUAL.

2. REMOVE BLANK SEAL FROM UNIT.

3. MEASURE YOUR SCOPE TO DETERMINE THE "NOMINAL EYE PIECE HEIGHT".

4. USING THE DIMENSIONAL DRAWING, DETERMINE WHAT HEIGHT YOUR 1/2" HOLES NEED TO BE. (IF THE DIMENSION NEEDED IS NOT SHOWN, CONTACT LABCONCO FOR ASSISTANCE)

5. PLACE BLANK SEAL AND TEMPLATE ON A SCRAP PIECE OF CARDBOARD. CENTER THE 1/2" ROUND HOLE PUNCH ON YOUR CENTER MARKS AND PRESS FIRMLY WITH A SLIGHT TWISTING MOTION. REPLACE SEAL ON UNIT.

6. IF YOU PREFER YOU CAN ORDER A PRE-PUNCHED SEAL FROM SCHEDULE BELOW.

SEE FULL SCALE TEMPLATE ON SHEET 2 OF 2

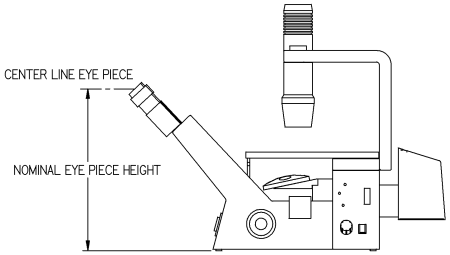

	SCHEDULE			
	LABCONCO P/N	PURE - VU EYE PIECE SEAL SIZE	NOMINAL EYE PIECE HEIGHT	FITS MICROSCOPE
	4027800	00	BLANK	ALL, SHIPS WITH UNIT
Not shown	4027810	10	XL OVERSIZED BLANK	ALL STEREO SCOPES (+/- 2.0" HEIGHT ADJUSTMENT), ZEISS DISCOVERY V8
Not shown	4027811	11	XL STEREO 16.0" (+/- 2.0")	NIKON SMZ 1500 STEREO, OLYMPUS SZX 16 STEREO, LEICA MZ95 STEREO
	4027813	13	13.0"	
	4027814	14	14.0"	ZEISS AXIOVERT 40 INVERTED
	4027815	15	15.0"	NYKON ECLIPSE TS100 INVERTED , OLYMPUS CKX31 INVERTED
	4027816	16	16.0"	LEICA DM IL LED INVERTED
	4027817	17	17.0"	LEICA DM 6000B DIGITAL

NOTE: Supplier of this part must ensure continued RoHS compliance

Signed certification will be requested periodically. Labconco Corporation reserves the right to return noncompliant parts at the vendor's expense. If you are unfamiliar with the RoHS standards, please contact Labconco for information.

DR BY jodell
DATE 07/20/09
CHKD BY (OPTIONAL)
DATE
TOLERANCES UNLESS OTHERWISE SPECIFIED
ANGULAR +1/2 DEG / INSIDE BEND RAD (1/16 / XX±.03 .XXX ± .010
REMOVE BURRS AND SHARP EDGES / DO NOT SCALE DWG

Protecting your laboratory environment
LABCONCO
LABCONCO CORPORATION, KANSAS CITY, MISSOURI 64132
(800) 821-5525, FAX (816) 363-0130, http://www.labconco.com

PRODUCT
PART NAME INSTRUCTION SHEET, MICROSCOPE SEAL
SHEET 1 OF 2
D 4027804 REV A

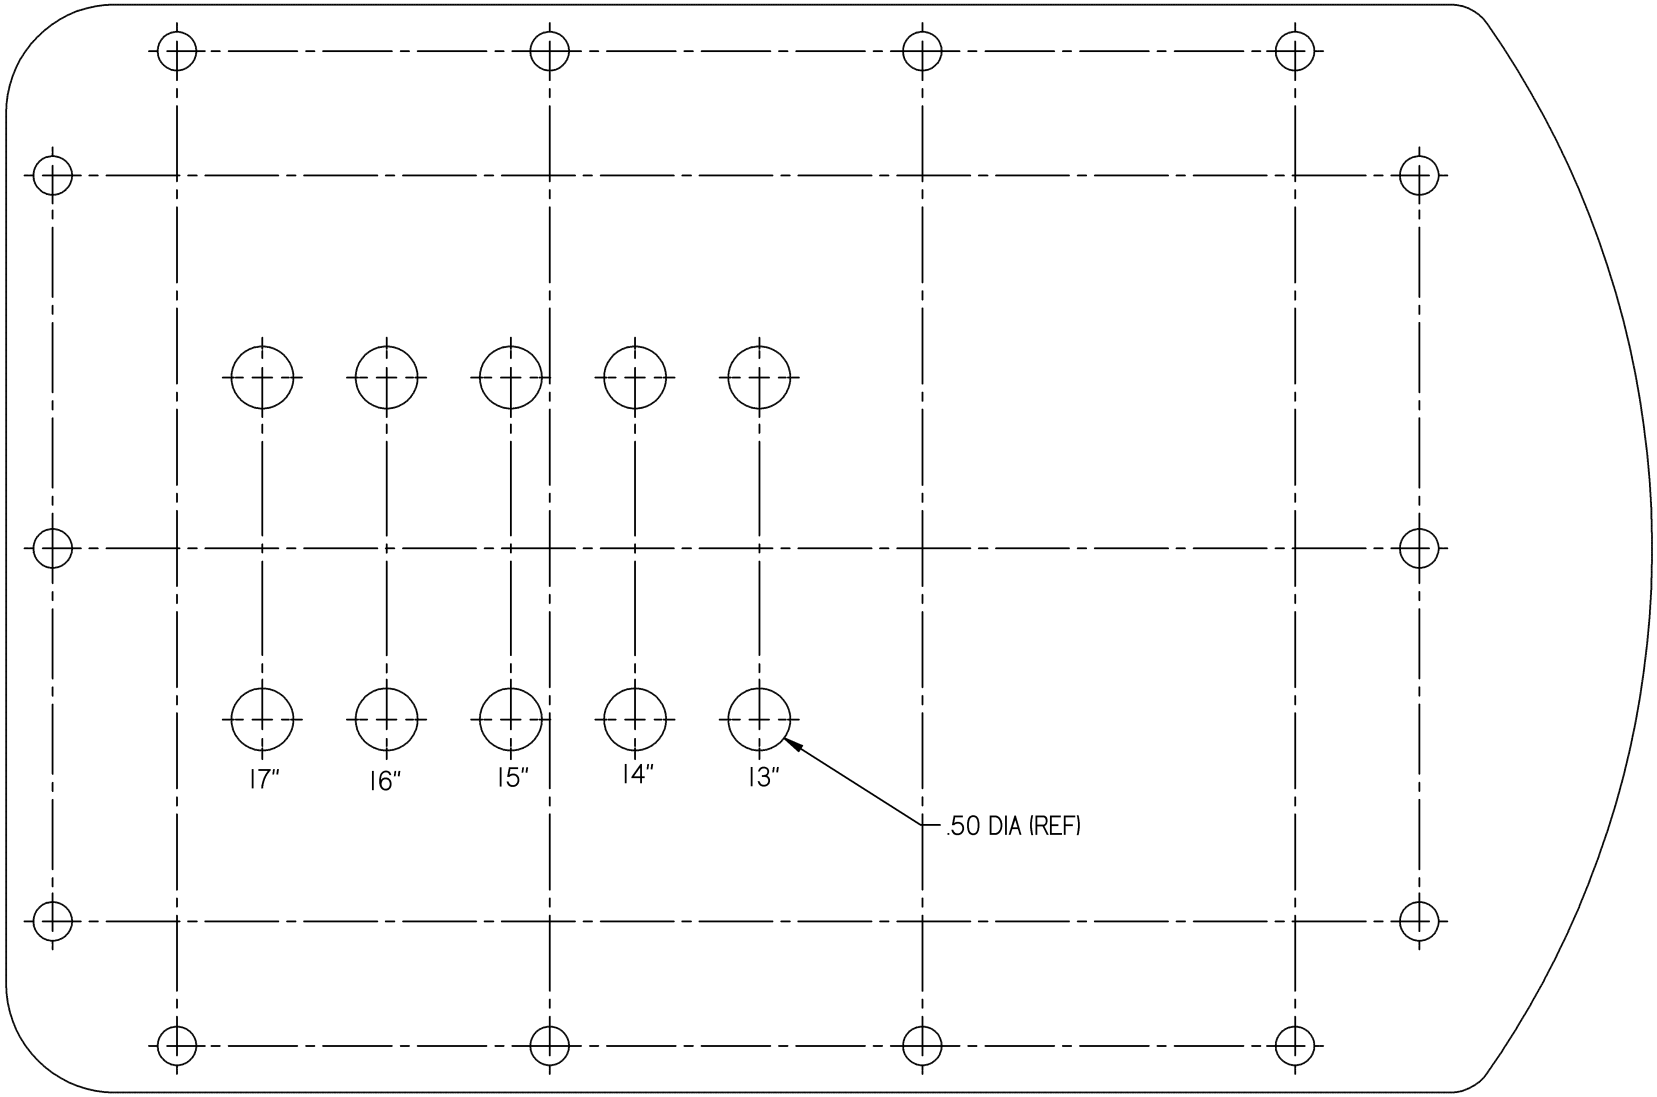

FULL SCALE TEMPLATE

4027804 REV. A SHT 2 OF 2